

Support Vector Machine Based Arrhythmia Classification Using Reduced Features

Mi Hye Song, Jeon Lee, Sung Pil Cho, Kyoung Joung Lee, and Sun Kook Yoo

Abstract: In this paper, we proposed an algorithm for arrhythmia classification, which is associated with the reduction of feature dimensions by linear discriminant analysis (LDA) and a support vector machine (SVM) based classifier. Seventeen original input features were extracted from preprocessed signals by wavelet transform, and attempts were then made to reduce these to 4 features, the linear combination of original features, by LDA. The performance of the SVM classifier with reduced features by LDA showed higher than with that by principal component analysis (PCA) and even with original features. For a cross-validation procedure, this SVM classifier was compared with Multilayer Perceptrons (MLP) and Fuzzy Inference System (FIS) classifiers. When all classifiers used the same reduced features, the overall performance of the SVM classifier was comprehensively superior to all others. Especially, the accuracy of discrimination of normal sinus rhythm (NSR), arterial premature contraction (APC), supraventricular tachycardia (SVT), premature ventricular contraction (PVC), ventricular tachycardia (VT) and ventricular fibrillation (VF) were 99.307%, 99.274%, 99.854%, 98.344%, 99.441% and 99.883%, respectively. And, even with smaller learning data, the SVM classifier offered better performance than the MLP classifier.

Keywords: Arrhythmia classification, linear discriminant analysis, reduction of feature dimension, support vector machine, wavelet transform.

1. INTRODUCTION

The electrocardiogram (ECG) remains the simplest non-invasive diagnostic method for determining various heart diseases. Physicians interpret the morphology of the ECG waveform and decide whether the heartbeat belongs to the normal sinus rhythm or to the class of arrhythmia.

Computerized electrocardiography is currently a well-established practice, supporting human diagnosis. Many algorithms have been proposed over previous years for developing the automated systems to

accurately classify the electrocardiographic signals in real-time [1-6]. Depending on the type used for the applied method of signal processing techniques and their formal description, we distinguish statistical, syntactic, or artificial intelligent methods [7].

Presently, artificial neural networks have particularly attracted attentions in the area of data processing. Many different neural solutions have been proposed [1-4]. The best known include the multilayer perceptron, the Kohonen self-organizing network, the fuzzy or neuro-fuzzy systems, and the combination of different neural networks within a hybrid system. Even though neural network is recognized as a powerful and promising technique for arrhythmia discrimination, it needs, however, to be learned with much data and has structural complexity. And, even though one of its competing systems, known as the fuzzy inference system, demands just simple computation without learning task, it requires the performance of repetitive experiments with the subjective opinion of specialists for setting membership functions.

In this paper, we proposed an algorithm for arrhythmia classification, which is associated with reduction of feature dimensions by linear discriminant analysis (LDA) and a support vector machine (SVM) based classifier. Since a SVM is known to have the advantage of offering solid performance of

Manuscript received March 10, 2005; revised July 2, 2005; accepted October 5, 2005. Recommended by Editorial Board member Moon Ki Kim under the direction of Editor Keum-Shik Hong. This work was supported by the Korea Health 21 R and D Project, Ministry of Health and Welfare, Republic of Korea under Grant 02-PJ3-PG6-EV08-0001.

Mi Hye Song, Jeon Lee, Sung Pil Cho, and Kyoung Joung Lee are with the Department of Biomedical Engineering, College of Health Science, Center for Emergency Medical Informatics (CEMI), Yonsei University, #217 Medical Industry Techno Tower Bldg. 1272 Maeji Ri, Heungup Myon, Wonju City, Kwangwon Do 220-842, Korea (e-mails: ohm9885@hotmail.com, {leejeon, saylas}@bme.yonsei.ac.kr, kjlee@dragon.yonsei.ac.kr).

Sun Kook Yoo is with the Department of Medical Engineering, Center for Emergency Medical Informatics, College of Medicine, Yonsei University, Seoul 120-752, Korea (e-mail: sunkyoo@yumc.yonsei.ac.kr).

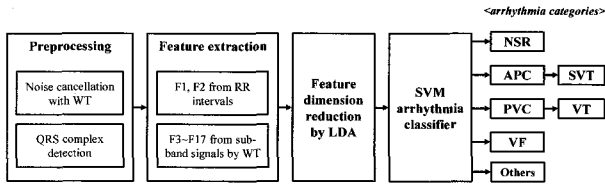


Fig. 1. Block diagram of proposed arrhythmia classifier.

classification with even smaller learning data, we can expect that the proposed algorithm, with relatively small learning data, would demonstrate better performance than other classifiers and be implemented faster on account of the reduction of feature dimensions. For a cross-validation procedure, this algorithm was compared with multilayer perceptrons (MLP) and fuzzy inference system (FIS) classifiers.

2. METHODS AND MATERIALS

2.1. Overview

The proposed algorithm includes preprocessing, feature extraction and feature dimension reduction by LDA and SVM based arrhythmia classification. Fig. 1 shows a block diagram of the proposed algorithm.


In this paper, the following arrhythmia categories have been considered: normal sinus rhythm (NSR), supraventricular tachycardia (SVT), arterial premature contraction (APC), ventricular tachycardia (VT), premature ventricular contraction (PVC) and ventricular fibrillation (VF).

For collecting arrhythmia data, we have used the ECG data from the MIT/BIH Arrhythmia Database digitized at a sampling rate of 360Hz. In addition, with the lack of VF data, Creighton University Ventricular Tachyarrhythmia Database and MIT-BIH Malignant Ventricular Arrhythmia Database, which had been sampled at 250 Hz, were resampled at 360 Hz and then used for VF.


The SVM classifier is the combination of NSR, APC, PVC, VF and other arrhythmia classifiers. The classification results of different classifiers form one output vector and the position of the highest value element of output vector indicates the membership with the appropriate class. Owing to the similar characteristics of the features of APC and SVT, their outputs of SVM are hardly distinguished. Opposed to APC, SVT is, however, inclined to occur in series. PVC and VT have much the same relationship. So, if output vector of said APC beat or PVC beat occurred more than three times consecutively, they were classified into SVT or VT respectively. Consequently, six types of arrhythmia were made to be classified by the proposed algorithm.

2.2. Preprocessing


Preprocessing is divided into noise cancellation,

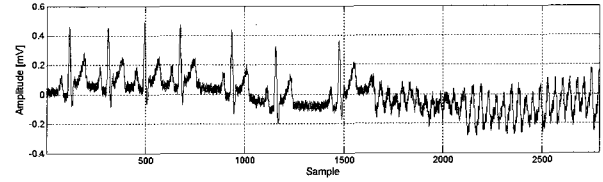


(a) Raw ECG signal.

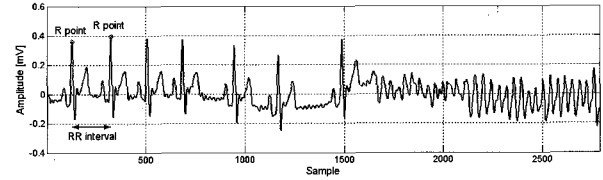

(b) Filtered ECG signal with WT.



(c) PSD of (a).



(d) PSD of (b).

Fig. 2. An example of raw ECG signal and filtered ECG signal.

QRS complex detection and beat segmentation for feature extraction and it cares about ECG signals sampled at 360 Hz. The wavelet transform (WT) has been verified as a good tool for preprocessing and QRS complex detection [8]. For the orthogonal wavelet transform, a discrete signal $x(n)$ can be expanded into the scaling function at j level as follows;

$$x(n) = D_j[x(n)] + A_j[x(n)], \quad (1)$$

where $D_j[x(n)]$ represents the detail signal at j level and $A_j[x(n)]$ represents the approximate signal at j level. Here, j level signifies the decomposition at scale 2^j . For noise cancellation such as baseline wander, 60 Hz interference and other high frequency noises, a filtered signal $x_f(n)$ is designed as

$$x_f(n) = A_2[x(n)] - A_8[x(n)]. \quad (2)$$

The corresponding bandwidth of the filtered signal is 0.7Hz to 45Hz for 360 Hz sampling rate. In Fig. 2, an example of raw ECG signal and filtered ECG signal are presented and cancellation of unnecessary high and low frequency noises can be found in time domain (Fig. 2(b)) and in frequency domain (Fig. 2(d)).

For the detection of the QRS complex, the wavelet transform based method, proposed by Park et al. [9], was used. For the filtered signal $x_f(n)$, the beat segment was defined to begin at 200 msec (= 72

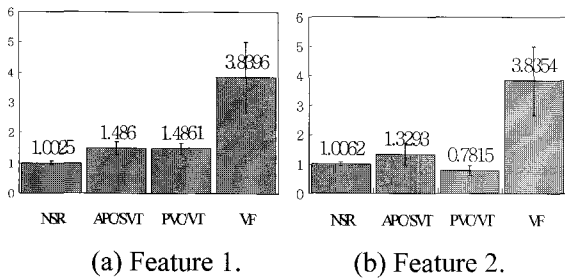


Fig. 3. The mean and variance of feature 1 and feature 2 for arrhythmia beats of 10 records from MIT/BIH arrhythmia database.

sample points) before R peak and to end at 200 msec after R peak so that it could have a total length of 400 msec. All considered features were extracted from this beat segment.

2.3. Feature extraction

The arrhythmias classification by neural network classifier requires generation of the input vectors. Since a physician classifies arrhythmia with the information of rhythm and morphology, an input vector should include features that represent the rhythm and morphology properly. Therefore, in this

paper, the input vector fed to the classifier was determined to be composed of 2 features related to rhythm, and 15 features related to morphology. If we define that $R(i)$ is the RR interval between present and just previous R peaks – an example is shown in Fig. 2(b), and K is a constant that corresponds to an RR interval that all men are generally expected to have, feature 1 and feature 2 can be calculated as

$$Feature\ 1 = \frac{K}{R(i)} \tag{3}$$

$$Feature\ 2 = \frac{K}{R(i+1)} \tag{4}$$

considering the sampling rate of 360 Hz, 300 sample points are chosen as K . The mean and variance of feature 1 and feature 2, which were calculated for four different classes (NSR, APC/SVT, PVC/VT and VF), are presented in Fig. 3. For these statistics, arrhythmia beats of 10 records from the MIT/BIH arrhythmia database are used.

In the mean time, morphology related features should satisfy that the differences among the ECG waveforms are suppressed for the waveforms of the same type but are emphasized for the waveforms

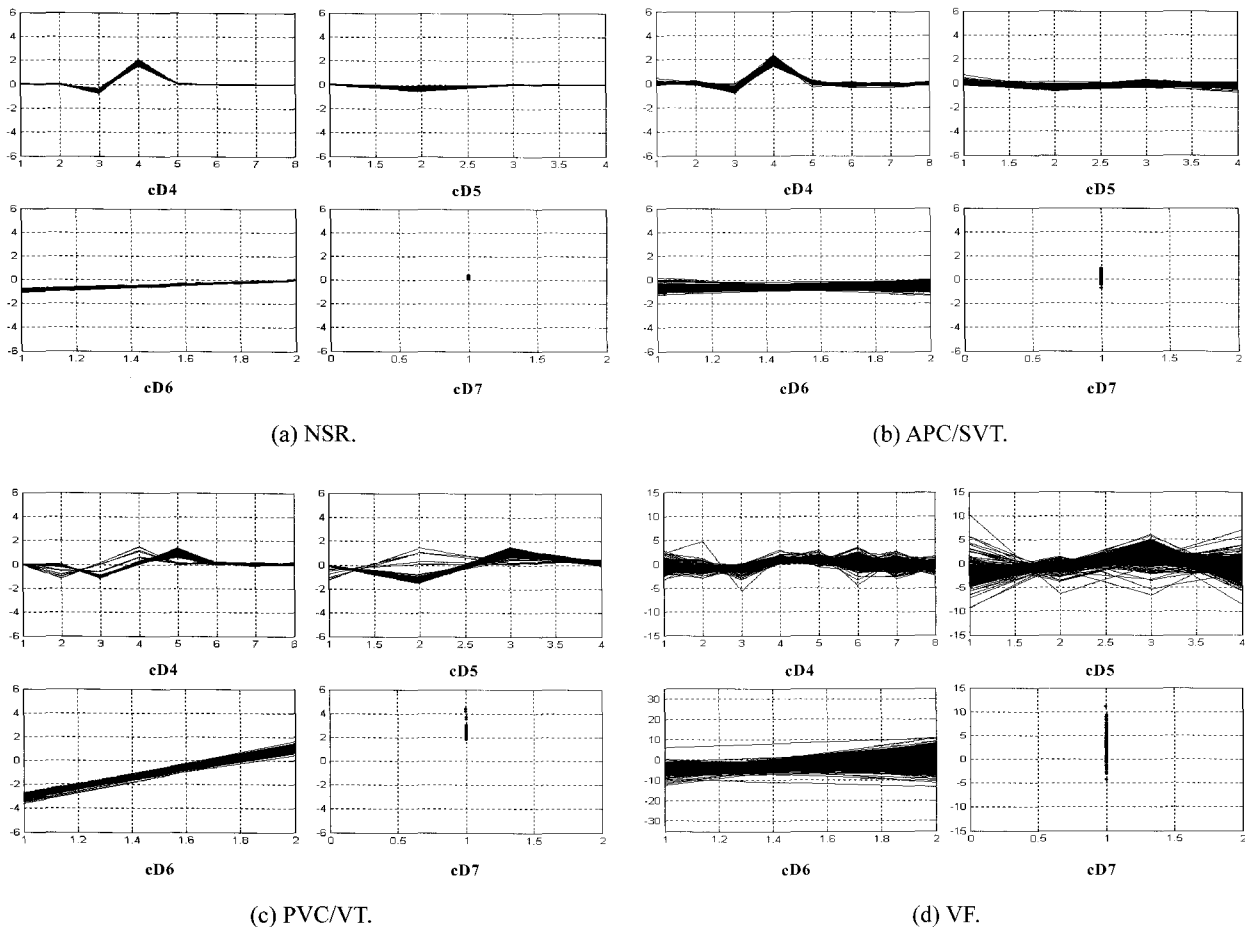


Fig. 4. The differences between detail coefficients' distributions for different types of beats.

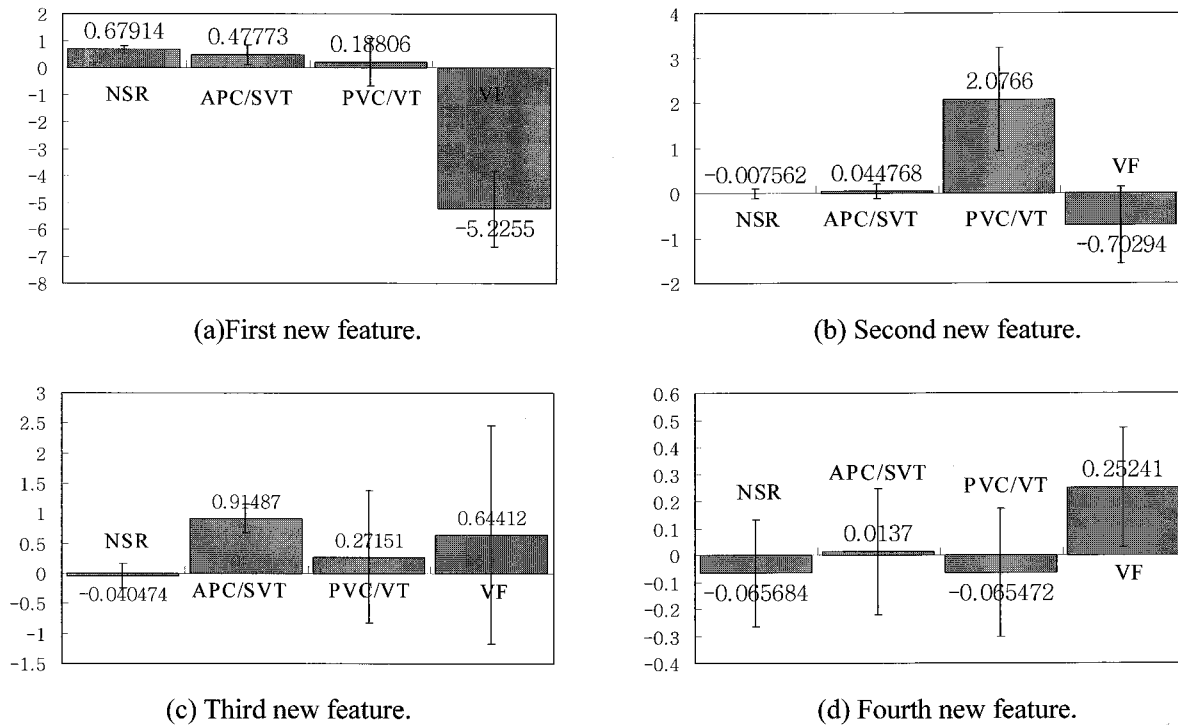


Fig. 5. Statistical characteristic of new features for arrhythmia beats of 10 records from MIT/BIH arrhythmia database for different classes.

belonging to different types of beats. Because it is difficult to separate one from the other on the basis of only time or frequency representation, sub-band signals by wavelet transform were utilized for morphology features. For NSR and interested types of arrhythmia, their detail signals at levels 4, 5, 6 and 7 have representative components and obviously different distributions to each other. Level 4 signifies the decomposition at scale 24. Based on these facts, detail coefficients of these detail signals were chosen as features that could discriminate arrhythmia beats from the others. The differences between detail coefficients' distributions for different types of beats can be found in Fig. 4. cD4 means that the detail coefficients at level 4 and the number of coefficients is 8. Similarly, cD5 at level 5, cD6 at level 6, cD7 at level 7 with the number of coefficients being 4, 2 and 1, respectively. These 15 coefficients were defined as feature 3 to feature 17.

2.4. Feature dimension reduction by LDA

Linear Discriminant Analysis (LDA) searches for those vectors in the underlying space that best discriminate among classes rather than those that best describe the data [10]. The goal of LDA is to seek a transformation matrix W that maximizes the ratio of the between-class scatter to the within-class scatter. Initially, we consider a within-class scatter matrix for the within-class scatter. A within-class scatter matrix S_w is defined as

$$S_w = \sum_{i=1}^c \sum_{x \in C_i} (x - m_i)(x - m_i)^t, \quad (5)$$

where c is the number of classes, C_i is a set of data belonging to the i th class, and m_i is the mean of the i th class. The within-class scatter matrix represents the degree of scatter within classes as a summation of covariance matrices of all classes. Next, we consider a between-class scatter matrix for between-class scatter. A between-class scatter matrix S_B is defined as

$$S_B = \sum_{i=1}^c (m_i - m)(m_i - m)^t, \quad (6)$$

where m is the mean of all classes. The between-class scatter matrix represents the degree of scatter between classes as a covariance matrix of means of all classes. We seek a transformation matrix W that in some sense maximizes the ratio of the between-class scatter and the within-class scatter. The criterion function $J(W)$ can be defined as

$$J(W) = \frac{|W^t S_B W|}{|W^t S_w W|}. \quad (7)$$

We can obtain the transformation matrix W as one that maximizes the criterion function $J(W)$. Furthermore, given a number of independent features relative to which data is described, LDA creates a linear combination of these which yields the largest mean

differences of the desired classes [11]. As a result, if there are c classes, the dimension of feature can be reduced to $c-1$ extremely. Using fewer inputs to the arrhythmia classifier, faster computation can be expected.

In this paper, assuming the number of classes is 5, the number of original features was designed to be reduced to 4 by LDA with guarantee of the comparable performance to that prior to reduction. The mean and variance of 4 features, which were newly generated by this process, are presented in Fig. 5. For different arrhythmia beats, their mean and variance are distributed in different ranges so that new features could also provide good tools for discrimination of arrhythmia beats.

2.5. SVM based arrhythmia classifier

The purpose of Support Vector classification is to devise a computationally efficient way of learning good separating hyperplanes in a high dimensional feature space. The SVM works in the high dimensional feature space formed by the nonlinear mapping, $\varphi(x)$ of the n -dimensional input vector into a K -dimensional feature space. The equation of the hyperplane separating two different classes is given by the relation

$$y(x) = W^T \varphi(X) = \sum_{j=1}^K \omega_j \varphi_j(x) + \omega_0 = 0 \quad (8)$$

with $w = [\omega_0, \omega_1, \dots, \omega_k]^T$ is the weight vector of the network.

By introducing the so-called Lagrange multipliers, α_i the learning task of SVM is reduced to quadratic programming. On account of these facts, there exist many highly effective learning algorithms [12-14], which result in the global minimum of the cost function and the best possible choice of the parameters of the neural network. And all operations in learning and testing are done using so-called kernel functions. The kernel is defined as $K(x, x_i) = \varphi^T(x_i)\varphi(x)$.

In this paper, a radial basis function (RBF) was selected as the kernel and the parameters - kernel width σ and margin-losses trade-off C , which provided best classification, were fixed by experiments before learning. Simultaneously, the learning of SVM can be referred to as the separation of learning vectors x_i into two classes of the destination values either $d_i=1$ or $d_i=-1$, with maximal separation margin. And this process is reduced to the dual maximization problem of the function, $Q(\alpha)$ defined as follows [12,15]:

$$Q(\alpha) = \sum_{i=1}^p \alpha_i - \frac{1}{2} \sum_{i=1}^p \sum_{j=1}^p \alpha_i \alpha_j d_i d_j K(x_i, x_j) \quad (9)$$

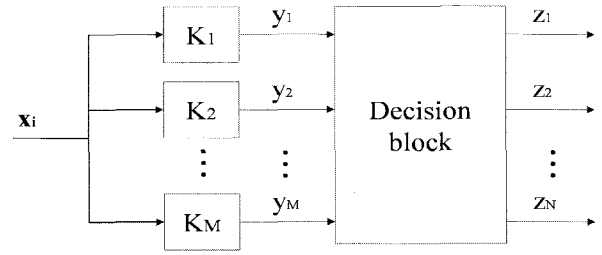


Fig. 6. The scheme of proposed SVM based classifier.

with the constraints

$$\sum_{i=1}^p \alpha_i d_i = 0, \quad 0 \leq \alpha_i \leq C, \quad (10)$$

where C is a user-defined trade-off constant as previously mentioned and p is the number of learning data pair (x_i, d_i) . C determines the balance between the complexity of the network, characterized by the weight vector w and the error of classification of data.

The solution with respect to the Lagrange multipliers gives the optimal weight vector W_{opt} , as $w_{opt} = \sum_{i=1}^{N_s} \alpha_{s_i} d_{s_i} \varphi(x_{s_i})$. The output signal $y(x)$ of the SVM network is determined as the function of

$$y(x) = \sum_{i=1}^{N_s} \alpha_{s_i} d_{s_i} K(x_{s_i}, x) + \omega_0 \quad (11)$$

kernels and the specific form of the nonlinear function need not be known. The positive value of $\varphi(x)$ is associated with membership of the particular class and the negative one with membership of the opposite class. Although SVM separates the data only into two classes, classification into additional classes is possible by applying either the ‘‘one against one’’ or: ‘‘one against all’’ method [16,17]. We designed a SVM based classifier as shown in Fig. 6.

The feature vectors x_i fed to the neural classifier K_j and the outputs of each classifier form the vector $y = [y_1, y_2, \dots, y_M]^T$ which signifies the potential of belonging to each class. Subsequently, with user-defined rules, output values y_j for some j may be inhibited and additional output may be generated through a decision block. As a result, final outputs $z = [z_1, z_2, \dots, z_N]^T$ are given. The position of the highest value element of z indicates the membership with the appropriate class.

3. RESULTS AND DISCUSSION

To evaluate the performance of the classifier, three measures are used and defined as:

$$Sensitivity(\%) = \frac{TP}{TP + FN} \times 100, \quad (12)$$

Table 1. Comparisons of the classifier performance for different combination of parameters.

| σ | $C=0.1$ | | |
|----------|-----------------|-----------------|--------------|
| | Sensitivity (%) | Specificity (%) | Accuracy (%) |
| 1 | 99.969 | 92.862 | 97.851 |
| 2 | 100 | 91.114 | 97.351 |
| 3 | 100 | 88.711 | 96.635 |
| 4 | 100 | 85.652 | 95.723 |
| σ | $C=1$ | | |
| | Sensitivity (%) | Specificity (%) | Accuracy (%) |
| 1 | 99.907 | 94.829 | 98.393 |
| 2 | 99.969 | 92.935 | 97.872 |
| 3 | 100 | 92.061 | 97.634 |
| 4 | 100 | 91.697 | 97.525 |
| σ | $C=10$ | | |
| | Sensitivity (%) | Specificity (%) | Accuracy (%) |
| 1 | 99.938 | 95.776 | 98.697 |
| 2 | 99.907 | 94.610 | 98.328 |
| 3 | 99.938 | 93.518 | 98.024 |
| 4 | 100 | 92.935 | 97.894 |

$$\text{Specificity}(\%) = \frac{TN}{TN + FP} \times 100, \quad (13)$$

$$\text{Accuracy}(\%) = \frac{(TP + TN)}{(TP + FN + TN + FP)} \times 100, \quad (14)$$

where TP stands for true positive, TN for true negative, FP for false positive and FN for false negative. When VF is concerned, TP represents VF being classified as VF and TN represents non-VF beat being classified as non-VF. Moreover, FP represents non-VF being misclassified as VF and FN represents VF being misclassified as non-VF [6].

3.1. Parameter selection

SVM classifier parameters, with kernel width σ and margin-losses trade-off C , affect the cost of learning and the classification performance. We have selected optimal parameter values with trial experiments, in which the performance of the classifier was observed for the different combination of parameters. For these experiments, the goal of the classifier was confined to discriminate only NSR with 10 records from the MIT/BIH arrhythmia database. Table 1 presents the

performance of the classifier corresponding to each experiment. The performance is likely to get lower as σ increases and the classifier has the better performance with $C=10$ than with other C s. So, we chose the parameters - σ and C as 1 and 10 respectively.

3.2. Feature dimension reduction by LDA

Two of the most popular dimensionality reduction techniques are Principal Component Analysis (PCA) and Linear Discriminant Analysis (LDA). The former one deals with the data in its entirety for the principal component analysis without paying any particular attention to the underlying class structure, whereas the latter one deals with discrimination between classes. To certify the usefulness of LDA, the performance of the classifier was evaluated with original features, features reduced to 4 dimensions by PCA and features reduced to 4 dimensions by LDA. For this, 23 records from the MIT/BIH arrhythmia database, which contain NSR and other types of arrhythmias, were used and the interested classes were confined as NSR and others. For this task, the SVM classifier was used with different input features and Multilayer Perceptrons (MLP) and the Fuzzy Inference System (FIS) were additionally tried with them for cross-validation. The results of classification are summarized in Table 2. ORG indicates the results with the original 17 features, PCA with 4 features by PCA and LDA with 4 features by LDA.

For the SVM classifier, the overall performance of PCA seems to be lower than that of ORG by less than 1%. In the mean time, the overall performance of LDA shows to be higher than both that of PCA and that of ORG. Even though other classifiers were used, the reduced features by LDA indicated usefulness for classification. Consequently, we found that the dimension of features had been reduced effectively by LDA and the better performance could be obtained with a smaller number of features than that of original features. Furthermore, faster learning was possible due to lower dimensions of input features.

3.3. Performance of SVM arrhythmia classifier

To verify the effectiveness of the SVM arrhythmia classifier, its performance was compared with that of well-known classifiers; Multilayer Perceptrons (MLP)

Table 2. Comparisons of the classifier performance for different feature reduction methods (units, %).

| | ORG | | | PCA | | | LDA | | |
|---------|-------------|-------------|----------|-------------|-------------|----------|-------------|-------------|----------|
| | Sensitivity | Specificity | Accuracy | Sensitivity | Specificity | Accuracy | Sensitivity | Specificity | Accuracy |
| MLP | 99.490 | 94.680 | 98.704 | 99.659 | 92.652 | 98.954 | 99.899 | 95.643 | 99.324 |
| FIS | 97.896 | 90.555 | 96.901 | 95.415 | 91.465 | 94.704 | 99.395 | 91.104 | 98.047 |
| SVM | 99.510 | 96.064 | 98.742 | 99.674 | 93.645 | 98.865 | 99.606 | 98.751 | 99.521 |
| Average | 98.966 | 93.766 | 98.116 | 98.249 | 92.587 | 97.508 | 99.633 | 95.166 | 98.964 |

Table 3. Comparisons of the performances with different classifiers (units, %).

| | MLP | | | FIS | | | SVM | | |
|----------------|-------------|-------------|----------|-------------|-------------|----------|-------------|-------------|----------|
| | Sensitivity | Specificity | Accuracy | Sensitivity | Specificity | Accuracy | Sensitivity | Specificity | Accuracy |
| NSR | 98.984 | 92.021 | 98.276 | 99.623 | 89.296 | 98.572 | 99.657 | 96.215 | 99.307 |
| APC | 85.185 | 100 | 98.374 | 80.574 | 100 | 98.374 | 88.294 | 99.951 | 99.274 |
| SVT | 84.706 | 100 | 99.148 | 81.345 | 100 | 99.148 | 82.821 | 100 | 99.854 |
| PVC | 93.085 | 97.9 | 97.505 | 89.754 | 99.362 | 98.377 | 92.157 | 98.937 | 98.344 |
| VT | 92.484 | 98.859 | 98.701 | 87.188 | 99.636 | 99.444 | 91.695 | 99.632 | 99.441 |
| VF | 99.341 | 99.958 | 99.903 | 99.254 | 100 | 99.934 | 99.751 | 99.993 | 99.883 |
| <i>Average</i> | 92.2975 | 98.123 | 98.651 | 89.623 | 98.049 | 98.975 | 92.396 | 99.121 | 99.350 |

and Fuzzy Inference System (FIS) classifiers.

For a MLP classifier, a three layer structure was used, including an input layer, a hidden layer and an output layer. Each input layer and output layer has 4 nodes and 5 nodes respectively. And, the hidden layer, using sigmoid functions as the membership functions, was made to have 10 nodes with best performance. The learning task was done by an error back propagation algorithm.

For a FIS classifier, input features were translated to linguistic values by the fuzzy inference, in which membership functions and fuzzy logic comprised of IF-THEN statements were used. A Gaussian curve was used for the membership functions, on which the performance of FIS is likely to be dependent, and its characteristic parameters were selected with repetitive experiments. A min-max method, also known as the Mandani inference method, was used for inference and a result was finally obtained by a gravity center defuzzification.

For the evaluation of each classifier, a total of 5630 beats were used and it consisted of 67438 NSR beats, 2318 APC and SVT beats, 8617 PVC and VT beats, 7175 VF beats and 82 other beats. All classifiers equally used 4 dimension features by LDA as input features. Table 3 shows the summarized results of cross-validation. The SVM classifier can discriminate NSR with accuracy of 99.307%, APC with 99.274%, SVT with 99.854%, PVC with 98.344%, VT with 99.441% and VF with 99.883%. The overall performance of the SVM classifier is generally better than that of the MLP classifier and that of the FIS classifier. And, the FIS classifier has the most inferior performance. This may be from the fact that the used features are not suitable for fuzzy inference and we could not find the best membership functions. For NSR and APC, the SVM classifier shows absolute superiority in all performance areas; sensitivity, specificity and accuracy. The sensitivity of the SVM classifier for NSR and VF is higher than that of the SVM classifier for other arrhythmias, for which MLP even demonstrate better sensitivity. And, the SVM classifier has mostly good specificity for all arrhythmias. The majority of errors are caused by

some arrhythmias not considered in this paper, such as LBBB (left bundle branch block), RBBB (right bundle branch block) and fusion beat. To obtain the above results, while the SVM classifier used 4135 beats in the learning task, the MLP classifier used 26512 beats, which is about six times more. Undoubtedly, when fewer beats were used for the MLP classifier, lower performances were obtained, but these are not shown here. Moreover, the CPU time taken to build the SVM classifier and MLP classifier were measured as 100.094 and 623.734 secs, respectively.

Finally, we can know that the proposed SVM classifier provides better performance than the MLP classifier with smaller learning data as well as than that of previous studies [1-6].

5. CONCLUSIONS

In this paper, we proposed a SVM based arrhythmia classification algorithm. Seventeen original input features were extracted from preprocessed signals by wavelet transform; 2 rhythm related features and 15 wavelet coefficient features. To improve the learning efficiency of the classifier, we attempted to reduce the original features to 4, the linear combination of original features, by LDA. Comparing the performance of the SVM classifier with different input features, the performance with features by LDA showed higher than with that by PCA and even with original features. So, we could see that LDA could reduce feature dimensions and act as a useful tool to improve the classifier performance at lower learning costs. To evaluate the SVM arrhythmia classifier, a cross-validation method was adopted. That is, the performance of it was compared with that of the MLP classifier and FIS classifier using dimension reduced features. The proposed SVM classifier showed satisfactory performances in discriminating six types of arrhythmia beats. The accuracy of discrimination of NSR, APC, SVT, PVC, VT and VF were 99.307%, 99.274%, 99.854%, 98.344%, 99.441% and 99.883%, respectively. The overall performance of the SVM classifier was comprehensively better than that of the

MLP classifier and the FIS classifier. And, even with smaller learning data, the SVM classifier could provide better performance than the MLP classifier.

Furthermore, the proposed algorithm could be expected to offer faster implementation than other neural networks by the reduction of feature dimensions by LDA and by less-demanding learning data characteristics of the SVM classifier.

REFERENCES

- [1] Y. H. Hu, S. Palreddy, and W. Tomkins, "A patient adaptable ECG beat classification using a mixture of experts approach," *IEEE Trans. Biomed. Eng.*, vol. 44, no. 9, pp. 891-900, September 1997.
- [2] Y. H. Hu, W. Tomkins, J. L. Urrusti, and V. X. Alfonso, "Applications of artificial neural networks for ECG signal detection and classification," *Electrocardiology*, vol. 24, pp. 123-129, 1994.
- [3] K. Minami, H. Nakajima, and T. Yoyoshima, "Real time discrimination of the ventricular tachyarrhythmia with Fourier-transform neural network," *IEEE Trans. Biomed. Eng.*, vol. 46, no. 2, pp. 179-185, 1999.
- [4] G. E. Oien, N. A. Bertelsen, T. Eftestol, and J. H. Husoy, "ECG rhythm classification using artificial neural networks," *Proc. of the IEEE Digital Signal Processing Workshop*, pp. 514-517, 1996.
- [5] T. Sugiura, H. Hirata, Y. Harada, and T. Kazui, "Automatic discrimination of arrhythmia waveforms using fuzzy logic," *Proc. of the IEEE Engineering in Medical and Biology Society*, vol. 20, no. 1, pp. 108-111, 1998.
- [6] L. Y. Shyu, Y. H. Wu, and W. Hu, "Using wavelet transform and fuzzy neural network for VPC detection from the Holter ECG," *IEEE Trans. Biomed. Eng.*, vol. 51, no. 7, pp. 1269-1273, 2004.
- [7] R. Schalkoff, *Pattern Recognition: Statistical, Structural and Neural Approaches*, Wiley, New York, 1992.
- [8] S. Kadambe, R. Murray, and G. F. B. Bartels, "Wavelet transform-based QRS complex detector," *IEEE Trans. Biomed. Eng.*, vol. 46, no. 7, pp. 838-848, July 1999.
- [9] K. L. Park, K. J. Lee, and H. R. Yoon, "Application of a wavelet adaptive filter to minimize distortion of the ST-segment," *Med. And Biol. Eng. and Computing*, vol. 36, no. 5, pp. 581-586, 1998.
- [10] H. C. Kim, D. J. Kim, and S. Y. Bang, "Face recognition using LDA mixture model," *Proc. of the Pattern Recognition*, vol. 2, pp. 925-928, 2002.
- [11] A. M. Martinez and A. C. Kak, "PCA versus LDA," *IEEE Trans. Pattern Analysis and Machine Intelligence*, vol. 23, no. 2, pp. 228-233, 2001.
- [12] A. Smola and B. Scholkopf, "A tutorial on support vector regression," *NeuroColt Tech. Rep. NV2-TR-1998-030*, Royal Holloway College, Univ. London, London, U. K., 1998.
- [13] O. L. Mangasarian, "Lagrangian support vector machines," *J. Machine Learning Res.*, vol. 1, pp. 161-177, 2001.
- [14] J. Platt, "Fast training of SVM using sequential optimization," *Advances in Kernel Methods-Support Vector Learning*, B. Scholkopf, C. Burges, and A. Smola, Eds. Cambridge, MIT Press, U.K., pp. 185-208, 1998.
- [15] C. Burges, "A tutorial on support vector machines for pattern recognition," *Knowledge Discovery and Data Mining*, U. Fayyad, Ed. Norwell, Kluwer, MA, pp. 1-43, 2000.
- [16] K. Crammer and Y. Singer, "On the learn ability and design of output codes for multi-class problems," *Proc. 13th Conf. Computational Learning Theory*, pp. 35-46, 2000.
- [17] C. W. Hsu and C. J. Lin, *A Comparison of Methods for Mmulti-class Support Vector Machines*, Nat. Taiwan Univ., Taiwan, 2000.



Mi Hye Song received the B.S. and M.S. degrees in Engineering from Yonsei University, Korea, in 2003, and 2005, respectively. Since 2005, she has been a Ph.D. student in the Biomedical Engineering Department at Yonsei University. Her research interests include ECG signal processing, digital signal processing, real-time system design, and medical instrumentation.




Jeon Lee received the B.S. and M.S. degrees in Engineering from Yonsei University, Korea, in 1996, and 1999, respectively. Since 1999, he has been a Ph.D. student in the Biomedical Engineering Department at Yonsei University. In 2005, he was awarded the Young Investigator Award at APCMBE05 sponsored by IFMBE. His research interests include nonlinear bio-signal processing, bio-impedance applications, mathematical modeling of cardiovascular circulation, measurement systems with wearable sensors, and others.




Sung Pil Cho received the B.S. and M.S. degrees in Engineering from Yonsei University, Korea, in 2001, and 2003, respectively. Since 2004, he has been a Ph.D. student in the Biomedical Engineering Department at Yonsei University. His research interests include biomedical signal processing, adaptive filter theory, and sleep

disorders.



Kyoung Joung Lee received the B.S., M.S., and Ph.D. degrees in Electrical Engineering from Yonsei University, Seoul, Korea, in 1981, 1983, and 1988, respectively. Since 1982, he has worked in Biomedical Engineering at Yonsei University. He was a Visiting Professor at Case Western Reserve University, Ohio, U.S.A. in 1993. He

is currently a Biomedical Engineering Professor at Yonsei University. His research interests include signal processing, cardiovascular modeling, cardiac diagnosis, and medical instrumentation.



Sun Kook Yoo received the B.S., M.S., and Ph.D. degrees in Electrical Engineering from Yonsei University, Seoul, Korea, in 1981, 1985, and 1989, respectively. He was an Assistant Professor of Electrical Engineering at Soonchunhyung University, from 1990 to 1994, and a Visiting Associate at the Department of Radiology, University

of Iowa, Iowa City, from 1998 to 2000. Currently, he is an Associate Professor in Medical Engineering, Yonsei University, and a Director of the Center for Emergency Medical Informatics (CEMI). His research interests include 3-D visualization, telemedicine, and real-time system design.